5 Depth Adjustable

Lancing Device With Ejector

Instructions for the Lancing Device

This Lancing Device With Ejector is used to obtain capillary whole blood samples needed for blood glucose monitoring or for other tests requiring one or two drops of blood. The Adjustable Tip on the Lancing Device allows you to choose the best depth of skin penetration. The ejector is more safe professional system for the lancet disposal. To obtain a drop of blood, first wash your hands with warm, soapy water. Dry your hands thoroughly before using the Lancing Device.

Sliding Barrel

Directions


- 1. Twist off the Lancing Device Cover.
- Insert a new Lancet firmly into the Lancet Carrier.
- 3 Hold the Lancet Needle Cover and gently twist it off of the Lancet.
- 4. Replace the Lancing Device Cover.
- **5** The Adjustable Tip offers 5 levels of skin penetration. To select the desired depth, twist the Adjustable Tip in either direction until the numbers line up with the Arrow.

To select the best depth: 1-2 for soft or thin skin

- 3 for average skin
- 4-5 for thick or calloused skin
- 6 Hold the Lancing Device Cover in one hand. Using the other hand, slowly pull the Sliding Barrel away from the Lancing Device Cover. You will hear a click, indicating that the Lancet Carrier is locked into position. Release the Sliding Barrel to return it to its original position.

Taking Care of Your Lancing Device With Ejector

Remove the Lancing Device Cover. Wash the Lancing Device Cover in warm, soapy water. Rinse well and allow it to dry thoroughly. Use alcohol or mild soap and water to wipe the remaining outside of the Lancing Device. The Lancing Device can be disinfected using 70% rubbing alcohol.(Hospitals should consult their own infection control protocols.)

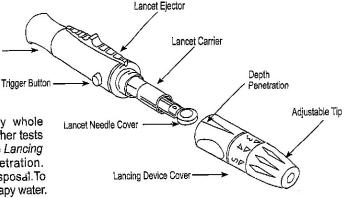

- Position the end of the Adjustable Comfort Tip against the side-tip of the finger. Press the Trigger Button, and then lift the Lancing Device away from the finger after the puncture is complete.
- 8 Place the Lancing Device aside and wait a few seconds for a blood drop to form. To help form a blood drop, lower the hand to waist level and gently massage the finger from palm to fingertip.
- To remove the used Lancet from the Lancing Device, first twist off the Lancing Device Cover. While holding the Sliding Barrel, leave the Lancet in the Lancet Carrier and firmly stick the Lancet Needle into the Lancet Needle Cover.
- Sliding the Lancet Ejector lever in a forward motion and disposing the used lancet in an approved container. Press the Trigger Button to release the Lancet Carrier. Replace the Lancing Device Cover. DO NOT re-use the Lancet. If the Lancing Device is to be used by another person, provide a new Lancing Device Cover and a new Lancet.

Limited Warranty

The Lancing Device will function effectively for a period of six (6) months from the date of purchase. A malfunctioning device should be returned to your supplier Supplie for replacement.